

عنوان آزمایش : Primidone

عنوان دستگاه : hplc

سری ساخت : 2-1400

عنوان کنترل :

شروع کنترل : 1400/02/28

پولد سرم


3SD	2SD	1SD	MEAN	-1SD	-2SD	-3SD	SD	CV%
6.481	5.984	5.487	4.99	4.493	3.996	3.499	0.497	9.963

تاریخ	مقدار
22/10/1400	5.4
25/10/1400	5.6
26/10/1400	5.3
27/10/1400	5.4
28/10/1400	5
29/10/1400	5.7
30/10/1400	5.1

تاریخ	مقدار
12/10/1400	5.5
13/10/1400	4.8
14/10/1400	4.4
15/10/1400	4.8
18/10/1400	5.2
19/10/1400	4.7
20/10/1400	5.4
21/10/1400	5.6

تاریخ	مقدار
01/10/1400	5.3
02/10/1400	5.3
04/10/1400	5.6
05/10/1400	5.3
06/10/1400	5.6
07/10/1400	5.9
09/10/1400	6.4
11/10/1400	5

Mean: 5.317	SD: 0.429	CV%: 8.072
-------------	-----------	------------

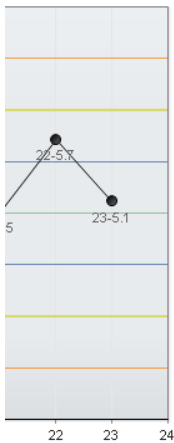

CV% 9.963 SD 0.497 -3SD 3.499 -2SD 3.996 -1SD 4.493 Mean 4.99 1SD 5.487 2SD 5.984 3SD 6.481



چاپ

عنوان کنترل

بولد سرم

اطلاعات

سری ساخت : 2-1400

آرشیو

شروع کنترل : 1400/02/28

مقدار تاریخ

5.3	1400/10/01
5.3	1400/10/02
5.6	1400/10/04
5.3	1400/10/05
5.6	1400/10/06
5.9	1400/10/07
6.4	1400/10/09
5	1400/10/11
5.5	1400/10/12
4.8	1400/10/13
4.4	1400/10/14
4.8	1400/10/15
5.2	1400/10/18
4.7	1400/10/19
5.4	1400/10/20
5.6	1400/10/21
5.4	1400/10/22
5.6	1400/10/25
5.3	1400/10/26
5.4	1400/10/27
5	1400/10/28
5.7	1400/10/29
5.1	1400/10/30

Mean: 5.317

SD: 0.429

CV%: 8.072

6σ

hplc

